


# NEW TOBACCO MOISTURE METER (Model : GMK-3306)

## 1. DESCRIPTION OF THE INSTRUMENT

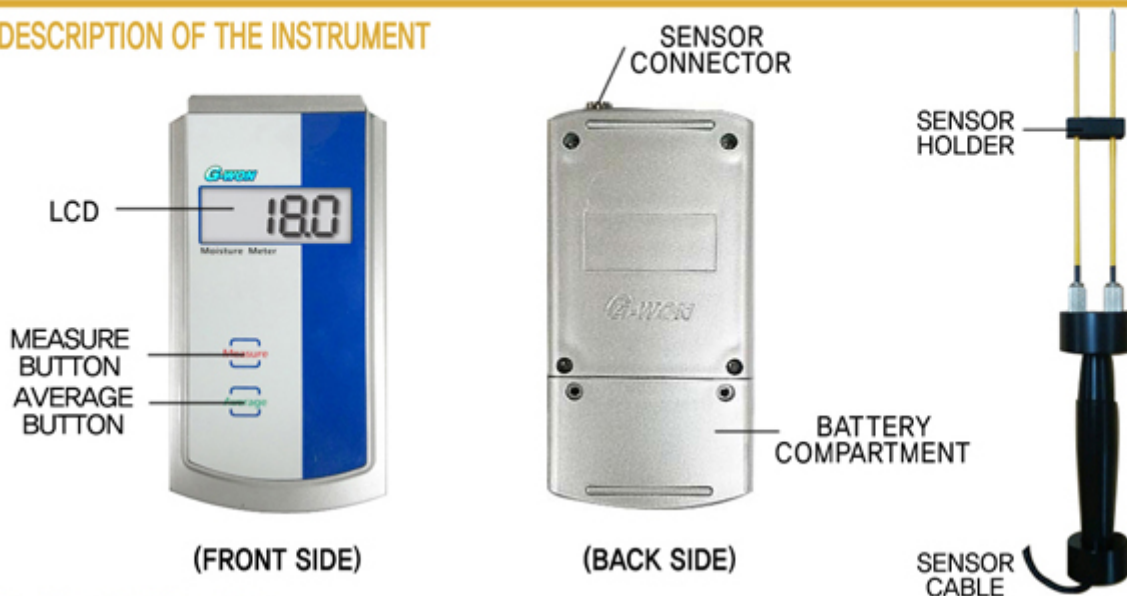

## 2. BEFORE MEASUREMENT

- CONNECT SENSOR CABLE WITH THE INSTRUMENT.
- WATCHING HOLES CAREFULLY, JOIN A 'SENSOR HOLDER' WITH TWO SENSOR PINS.
- OPEN THE LID OF BATTERY COMPARTMENT (BACK SIDE) AND PLACE 9V BATTERY 1EA IN IT.
- 'F06' SIGN APPEARS ON LCD AND DISAPPEARS, THE INSTRUMENT IS READY TO MEASURE IN NOMAL CONDITION (AUTO CALIBRATION).

## 3. MEASUREMENT

- PREPARE FOR THE TEST SAMPLE AND PLACE AN INSTRUMENT AT THE SAME PLACE FOR ABOUT 10 MINUTES.
- INSERT TWO SENSORS (WHIT SENSOR HOLDER) INTO THE BUNDLE OF TOBACCO LEAVES STRAIGHTLY.
- PRESS 'MEASURE' BUTTON, AND THE MEASUREMENT RESULT APPEARS ON LCD FOR ABOUT ONE MINUTE.  
(# WHEN THE MOISTURE % OF THE TEST SAMPLE IS BELOW 11%, "ErL" SIGN APPEARS AND IN CASE OF OVER 40%, "ErH" SIGN APPEARS.)
- PRESS 'AVERAGE' BUTTON, AND YOU CAN GET THE AVERAGE DATA (UP TO 9 TIMES).
- PRESS 'AVERAGE' BUTTON ONE MORE TIME, THE POWER IS OFF.
- WHEN THERE IS NO OTHER OPERATION, THE POWER IS OFF AUTOMATICALLY AFTER 3 MINUTES (AUTO HOLD & AUTO OFF FUNCTION).

## 4. IMPORTANT

- DO NOT STORE THE INSTRUMENT AT DAMP PLACE.
- IN CASE OF NO USE FOR A LONG TIME, MAKE SURE TO REMOVE THE BATTERY.
- THE MANUFACTURER GRANTS A TOTAL REPLACEMENT WARRANTY OF 12 MONTHS AFTER THE DATE OF PURCHASE.
- IN CASE OF WRONG USE, ABUSE OR MISUSE, WARRANTY WILL NOT AVAILABLE.

## G-WON HITECH CO., LTD.

WOOLIM E-BIZ. CENTER 310,  
#170-5, GURO-DONG, GURO-GU,  
SEOUL, KOREA(152-769)  
Tel : 82-2-2108-1646(DIR.)  
Fax : 82-2-2108-1649  
E-MAIL: g-won@g-won.co.kr

### Other Instruments

- |                        |                         |
|------------------------|-------------------------|
| ■ Grain Moisture Meter | ■ Coffee Moisture Meter |
| ■ Wood Moisture Meter  | ■ Digital Refractometer |
| ■ Flour Moisture Meter | ■ Soil Moisture Meter   |
| ■ Tea Moisture Meter   | ■ Fruit Acidity Meter   |

